


Add investigational value to the
rtx1™ AO Retinal Camera




AOdetect™

Segmentation software for
Adaptive Optics images

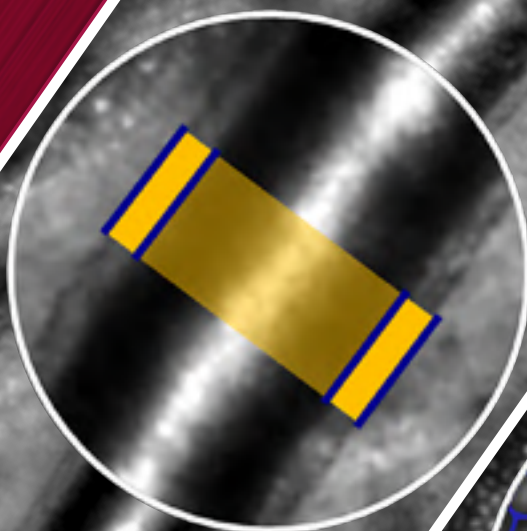

Walls

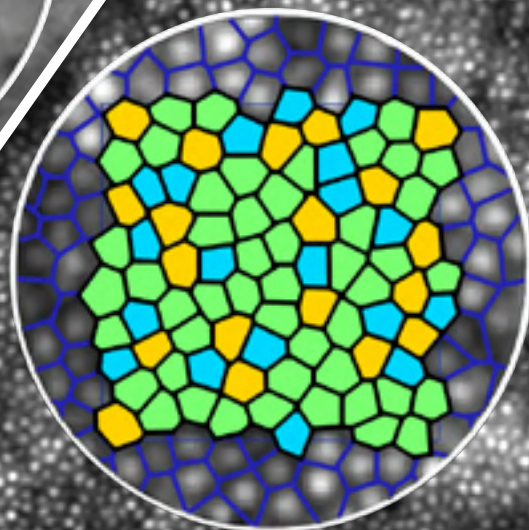


Mosaic

AOdetect™

Segmentation application for rtx1™ Adaptive Optics Retinal Images

Adopted by rtx1 users to analyze AO retinal images

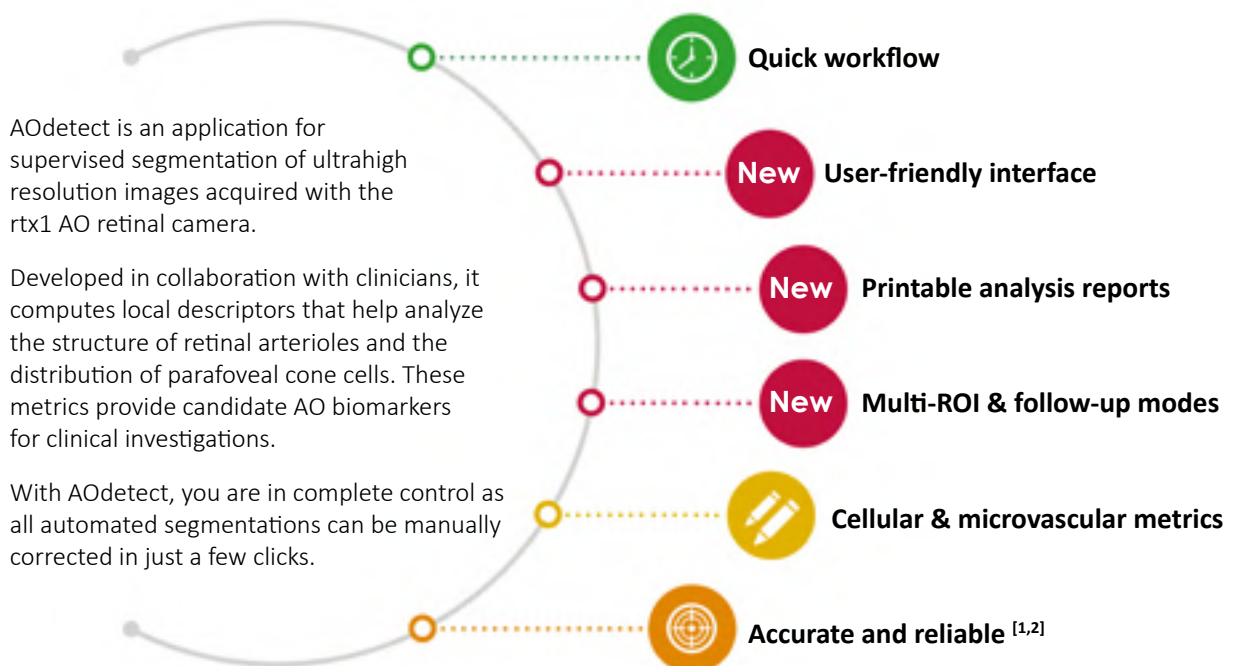

rtx1 + AOdetect : Fast follow-up workflow


Thanks to its high-precision algorithm, the rtx1 delivers follow-up AO images that are perfectly aligned with the baseline image.

AOdetect enables analyzing the exact same region in baseline and follow-up images, with only a few clicks.

New

Your follow-up analysis is automatically updated with each new visit.

This is how you can easily monitor a specific group of cells or chosen vascular section over time.

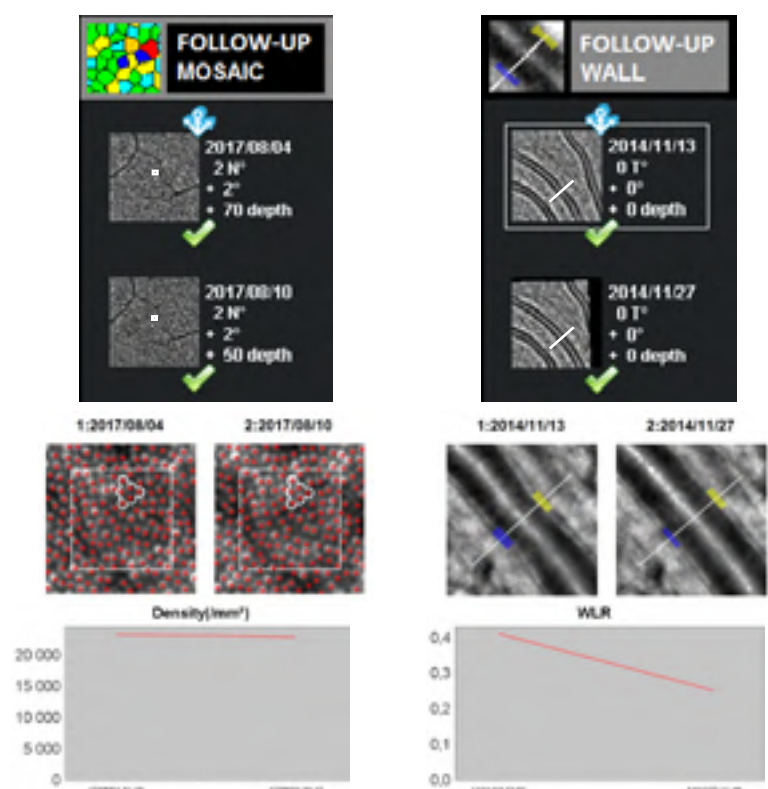

Wall

For images of small retinal arteries

Automated wall segmentation and thickness computation

Manual correction : click-and-drag to displace the wall borders while monitoring their position in the gradient profile


Wall metrics

- Internal and external diameter
- Wall thickness
- Wall Cross Section Area (WCSA)
- Wall to Lumen Ratio (WLR)

Reproducibility

0.7% for internal diameter ^[1]

3.3% for Wall to Lumen Ratio ^[1]

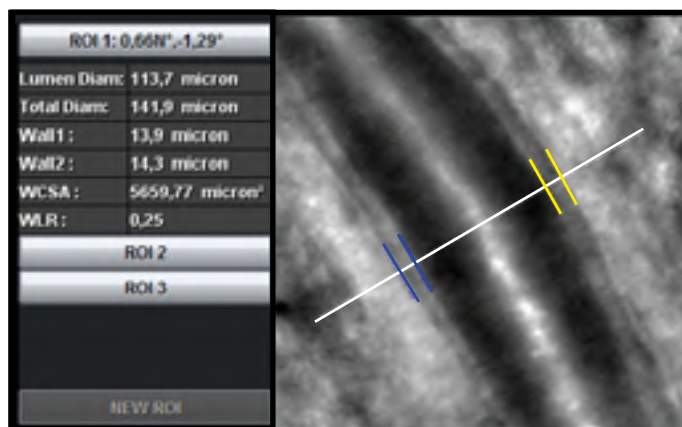

Example of analysis results in metric units. Visual units are also available.

Mosaic

For images of parafoveal cone cells

Automated mosaic segmentation and Voronoi analysis

Manual correction : simple clicks to add and remove cells while monitoring the Voronoi segmentation

Mosaic metrics


- Cell density
- Inter-cell spacing
- Regularity index
- Dispersion index

Reproducibility


4% for cell density ^[2]

Color-coded Voronoi diagrams

- Density
- Spacing
- Regularity

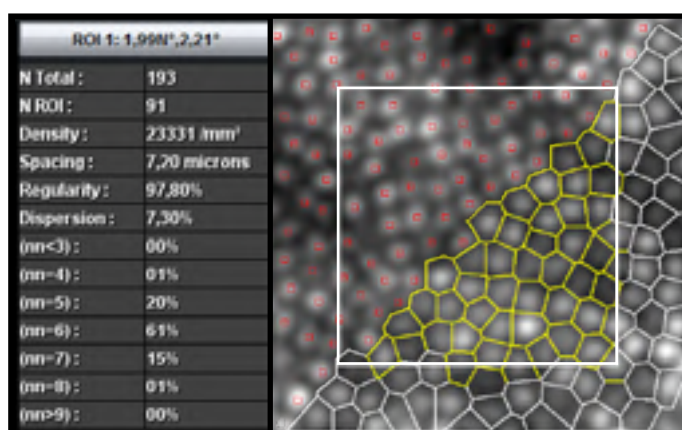

Example of analysis results in metric units. Visual units are also available for reduced variability in Voronoi cell density and inter-cell spacing^[2].

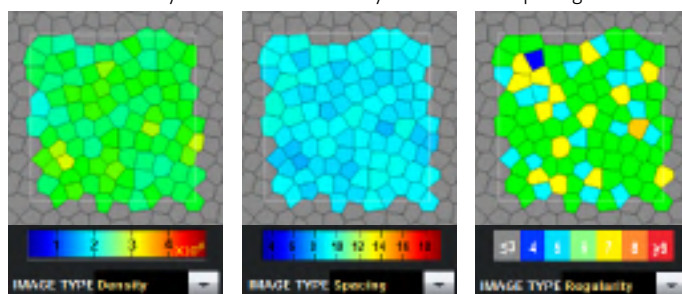

AOdetect interface and reports

New

” The retinal image analysis with rtx1 offers a novel noninvasive measurement of early changes in the vasculature that are not detectable on routine clinical examination.

Zaleska-Żmijewska et al. *J Diab Research*, 2017

” In arterial hypertension, WLR is a robust, dimensionless parameter that can be measured on large cohorts of nondilated patients.

Paques et al., *Prog Ret Eye Research*, 2018


” The rtx1 retinal image evaluation demonstrated photoreceptors loss in DM1 diabetic patients prior to any clinical changes.

Cristescu et al. *Rom J Ophthalmol*, 2019


” AO images showed a decrease in the number of foveal cone densities over 2 years in patients with RP. AO may shorten the period required to predict the RP progression rate.

Ueda-Consolvo et al. *Graefes Arc Clin Exp Opht*, 2019


Walls x Multi-ROI

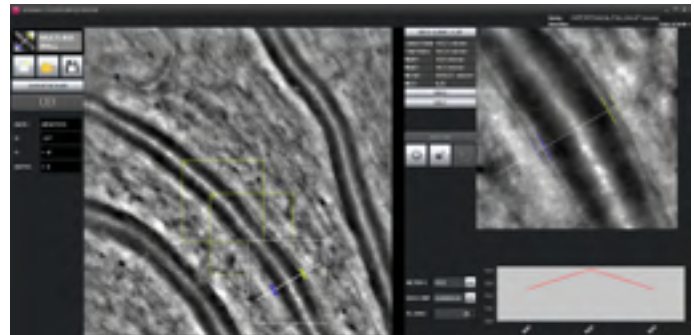


Walls x Multi-ROI Report

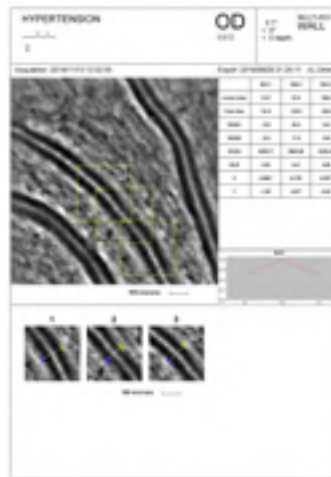

Mosaic x Follow-up Report

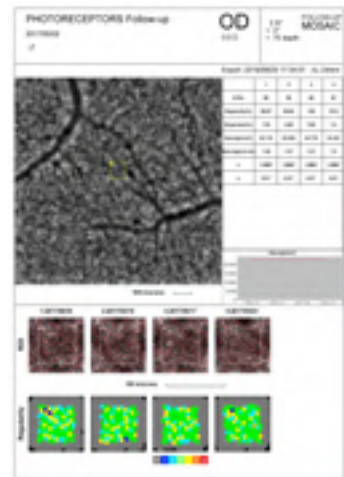

Mosaic x Follow-up

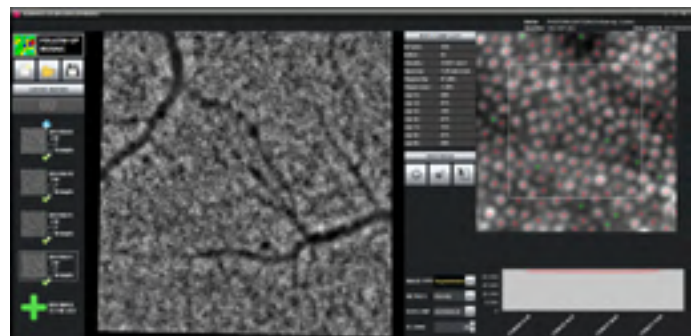

SPECIFICATIONS

Computer requirements

OS
RAM
CPU

Export formats
Analysis results
Printable reports

AOdetect Software

Windows XP-SP3, 7-SP1, 10
4 Gbyte or more
Intel i3 or higher

Text file
JPEG



AOdetect is an option of the certified rtx1 device in the European Union. In other territories, AOdetect is a separate product for research use only.

For use by trained eyecare professionals only.



18 rue Charles de Gaulle, 91400 Orsay, FRANCE

Contact number in Paris, FRANCE :
+33 (0) 1 64 86 15 66

Contact number in San Francisco, CA, USA :
+1 (415) 944-4461

contact@imagine-eyes.com
www.imagine-eyes.com